


TEST REPORT

(Electronic version)

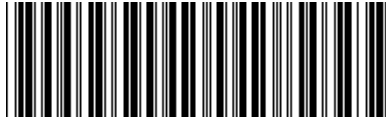

No:200131347

VERIFICATION WEBSITE: www.gttc.net.cn

VERIFICATION CODE: UFIQ-5533-34

扫码下载报告



ISSUE DATE:2020-06-04

APPLICANT: HUBEI WANFUL PROTECTIVE PRODUCTS CO., LTD.
ADDRESS: NO.113 MIAN YANG DA DAO XIANTAO CITY, HUBEI PROVINCE, CHINA

INFORMATION CONFIRMED BY APPLICANT:

DISPOSABLE FACE MASK

QUANTITY: 40 PIECES

COLOUR: BLUE

DATE RECEIVED/DATE TEST STARTED: 2020-05-18

CONCLUSION:

FILTRATION EFFICIENCY	M
INSPIRATORY RESISTANCE	M
EXPIRATORY RESISTANCE	M

NOTE: "M" -MEET THE STANDARD'S REQUIREMENT "F" -FAIL TO MEET THE STANDARD'S REQUIREMENT
"---" -NO COMMENT

REMARK:

THIS REPORT IS THE ENGLISH TRANSLATION VERSION OF THE REPORT 200131346.
ALL THE TESTED ITEMS ARE TESTED UNDER THE STANDARD CONDITION (EXCEPT FOR INDICATION).
COPIES OF THE REPORT ARE VALID ONLY RE-STAMPED.
THE EXPERIMENT WAS CARRIED OUT AT No.1, ZHUJIANG ROAD, PANYU DISTRICT, GUANGZHOU, GUANGDONG, P. R. CHINA.

APPROVED BY:

ZiShan Guo SENIOR ENGINEER

郭子山




PAGE 1 OF 3

TEST REPORT

(Electronic version)

No:200131347

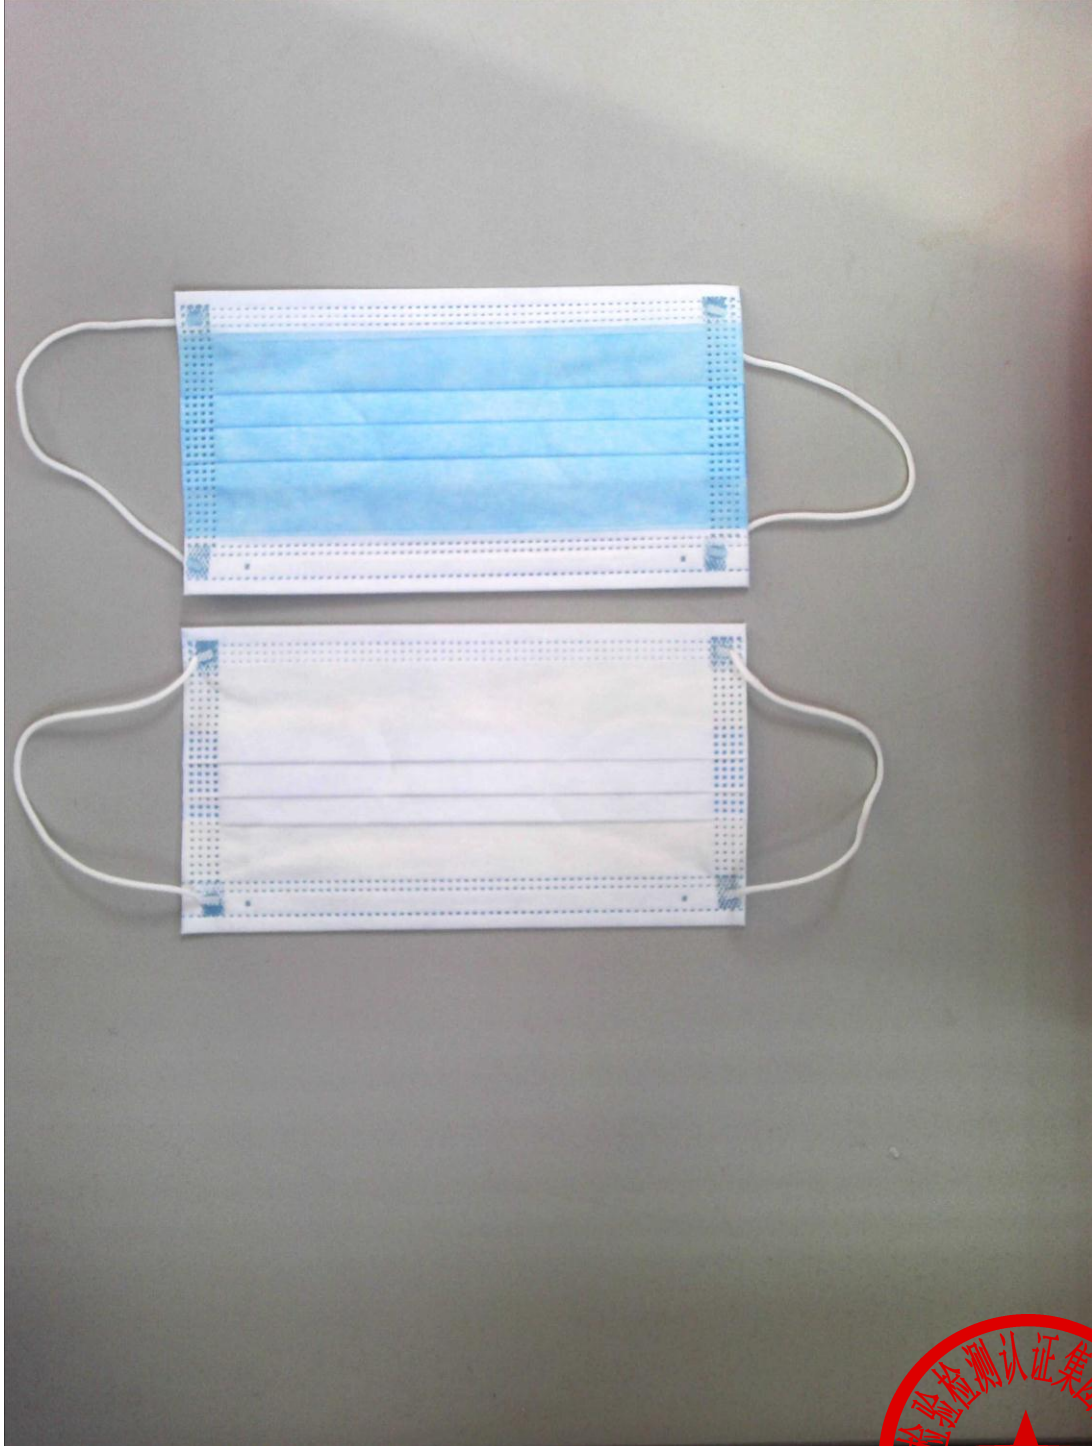

TEST REPORT

(Electronic version)

No:200131347

FILTRATION EFFICIENCY (%)

(GB/T 32610-2016 ANNEX A, AIR FLOW:85L/min, AEROSOL:NaCl, AEROSOL CONCENTRATION:15mg/m³, TEMP:24.7°C, RH:35.3%)

SALT MEDIUM:
MINIMUM 97.2

REQUIREMENT
SALT MEDIUM:
≥90
(GRADE III)
(GB/T 32610-2016)

INSPIRATORY RESISTANCE (Pa)

(GB/T 32610-2016 6.7, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
1# 124.8
2# 133.1
PRETREATMENT SAMPLE:
1# 115.3
2# 114.4

REQUIREMENT
≤175
(GB/T 32610-2016)

EXPIRATORY RESISTANCE (Pa)

(GB/T 32610-2016 6.8, HEAD SIZE: MEDIUM)

UNTREATED SAMPLE:
1# 103.2
2# 115.4
PRETREATMENT SAMPLE:
1# 89.4
2# 80.6

REQUIREMENT
≤145
(GB/T 32610-2016)



—End of Report—

PAGE 3 OF 3